



FLUKE®

Fluke 5820A Oscilloscope Calibrator Specifications

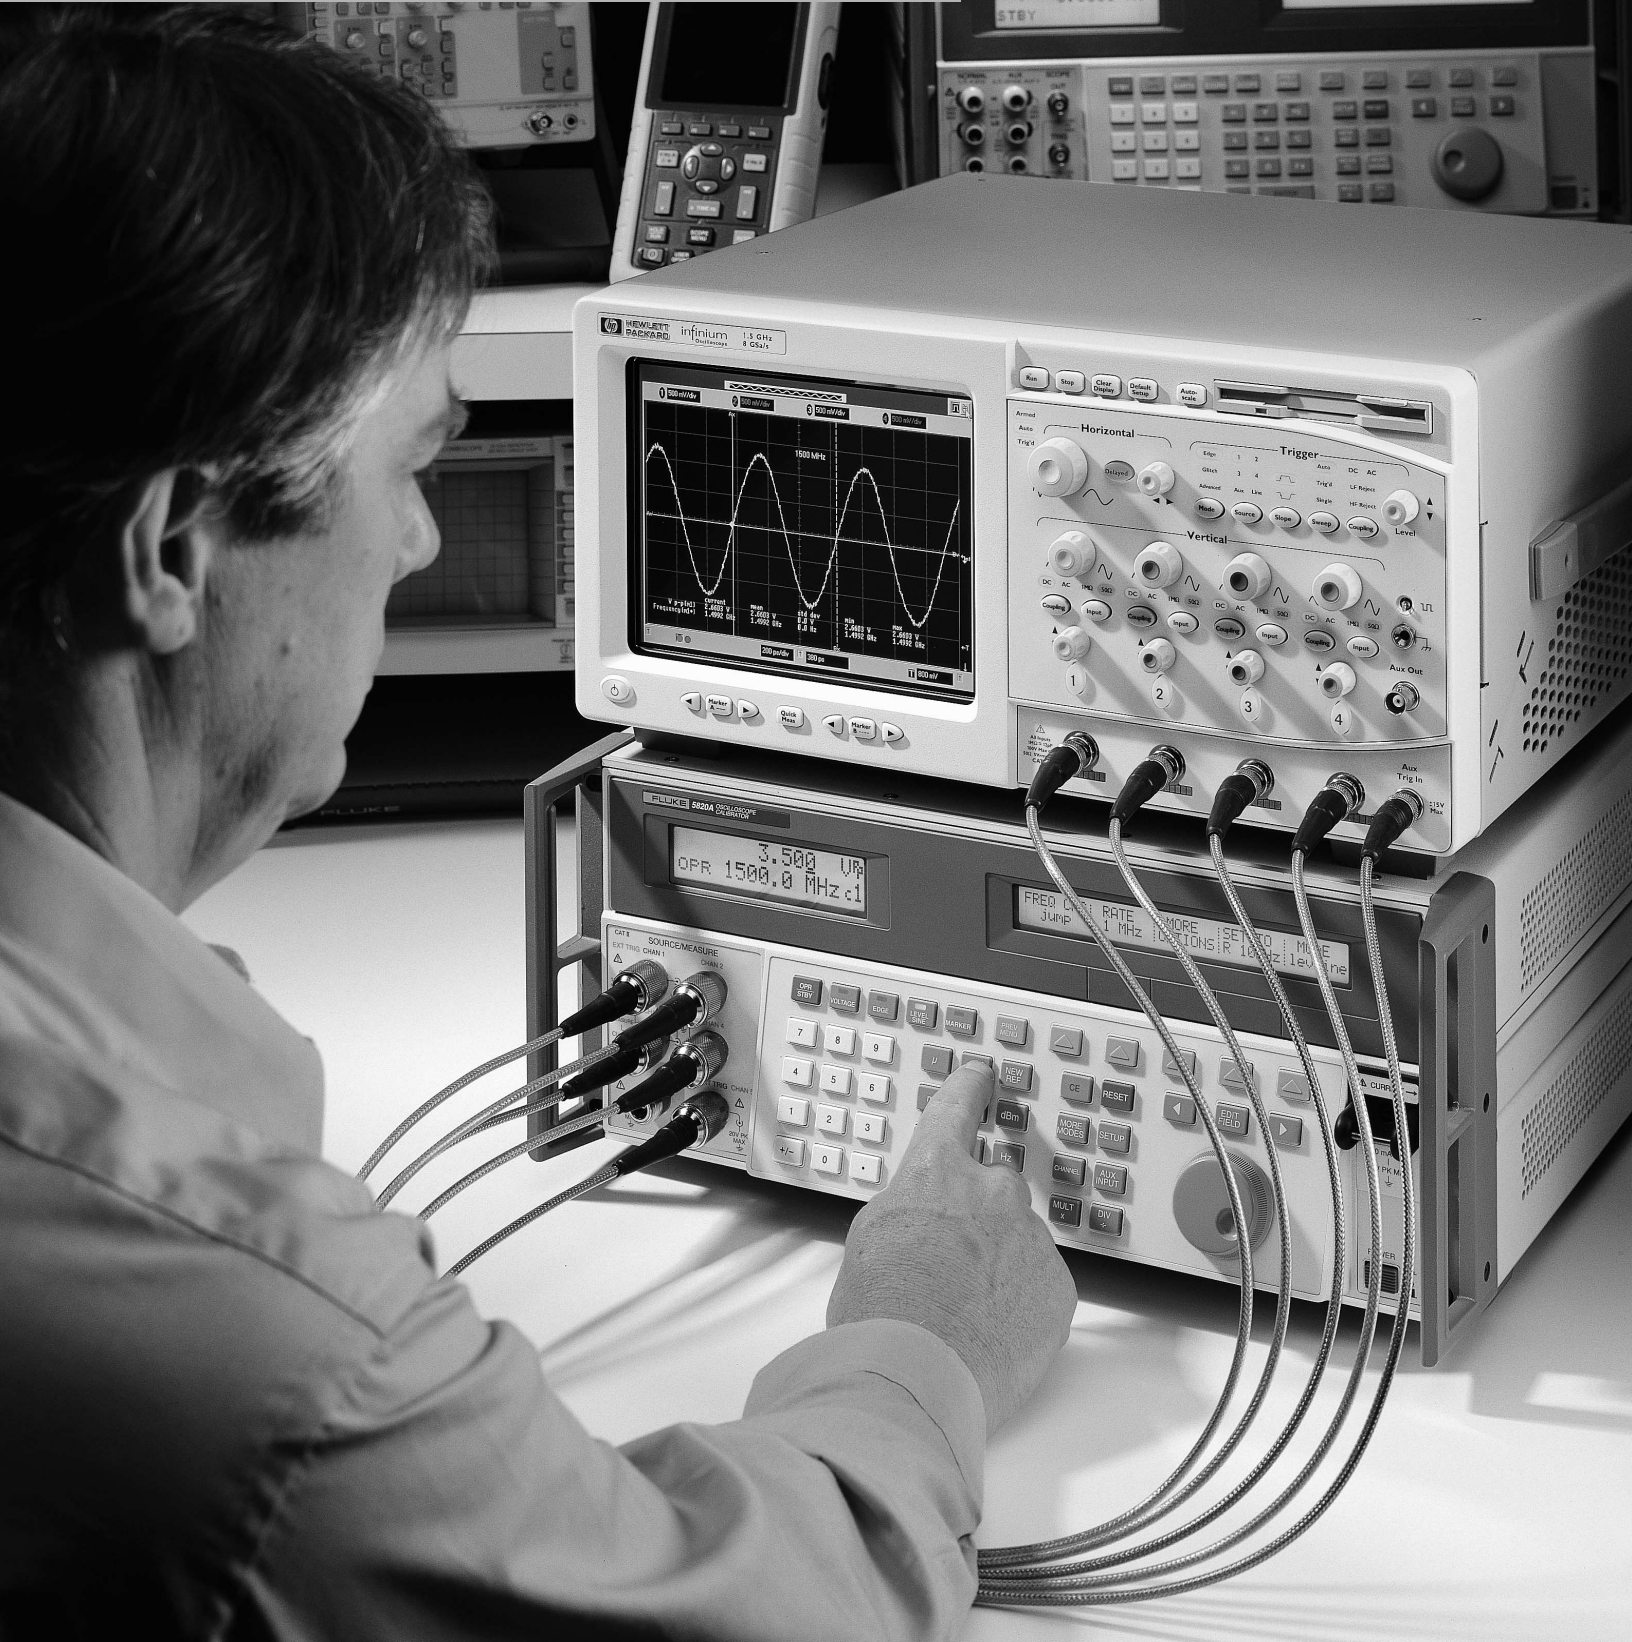

HP Hewlett-Packard Infinium 1.5 GHz 8 GS/s

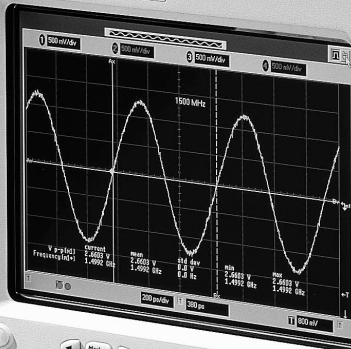

FLUKE 5820A OSCILLOSCOPE CALIBRATOR
3.500 Vp
OPR 1500.0 MHz c1

FREQ CH1 RATE MORE SET/NO MORE
Jump 1 MHz 1000000 Hz 1000000 Hz

CH1 SOURCE MEASURE
EXT TRIG CHAN1 CHAN2
TRIG CHAN1 TRIG CHAN2
VOLTAGE LOCK LINK TRACE MARKER
NEW DEL
dBm
Hz
MORE ACCESS SETUP
CHANNEL AUX INPUT
MULT X DIV

Voltage Function

Volt Function	DC Signal		Square Wave Signal ¹	
	into 50Ω	into 1 MΩ	into 50Ω	into 1 MΩ
Amplitude Range	0V to ±6.6V	0V to ±130V	± 1 mV to ±6.6V p-p	± 1 mV to ±130V p-p
1-Year Absolute Uncertainty, tcal ±5°C	± (0.25% of output + 40 μV)	± (0.025% of output + 25 μV)	± (0.25% of output + 40 μV)	± (0.05% of output + 5 μV)
Sequence	1-2-5 (e.g., 10 mV, 20 mV, 50 mV)			
Frequency Range	10 Hz to 10 kHz			
1-Year Absolute Uncertainty, tcal ±5°C	±(0.33 ppm of setting)			

¹ Positive or negative, zero referenced square wave.

Edge Function

Edge Characteristics into 50Ω	1-Year Absolute Uncertainty, tcal ±5°C
Amplitude Range (p-p)	4.0 mV to 2.5V ± (2% of output + 200 μV)
Frequency Range	1 kHz to 10 MHz ± (0.33 ppm of setting)
Rise Time	≤300 ps +0/-100 ps
Typical Jitter, edge to trigger	<3 ps (p-p) •
Leading Edge Aberrations	within 2 ns from 50% of rising edge < (3% of output + 2 mV)
	2 ns to 5 ns < (2% of output + 2 mV)
	5 ns to 15 ns < (1% of output + 2 mV)
	after 15 ns < (0.5% of output + 2 mV)

Fast Edge Function (2.1 GHz Option)

Edge Characteristics into 50Ω	1-Year Absolute Uncertainty, tcal ±5°C
Amplitude Range (p-p)	250 mV
Frequency Range	1 kHz to 100 kHz ± (0.33 ppm of setting)
Rise Time	≤150 ps +0/-25 ps

Leveled Sine Wave Function ≤600 MHz

Leveled Sine Wave Characteristics into 50Ω	Frequency Range				
	50 kHz (reference)	50 kHz to 100 MHz	100 MHz to 300 MHz	300 MHz to 500 MHz	500 MHz to 600 MHz
Amplitude Range (p-p)	5 mV to 5.5V				
1-Year Absolute Amplitude Uncertainty, tcal ±5°C	± (2% of output + 300 μV)	± (3.5% of output + 300 μV)	± (4% of output + 300 μV)	± (5.5% of output + 300 μV)	± (6% of output + 300 μV)
Flatness (relative to 50 kHz)	Not applicable	± (1.5% of output + 100 μV)	± (2% of output + 100 μV)	± (3.5% of output + 100 μV)	± (4% of output + 100 μV)
Short-term Amplitude Stability	≤1% ¹				
Frequency Resolution	10 kHz				
1-Year Absolute Frequency Uncertainty, tcal ±5°C	±0.33 ppm				
2nd Harmonic	≤-33 dBc				
3rd and Higher Harmonics	≤-38 dBc				

¹ Within one hour after reference amplitude setting, provided temperature varies no more than ±5°C.

Leveled Sine Wave Function >600 MHz (2.1 GHz Option)

Leveled Sine Wave Characteristics into 50Ω	Frequency Range			
	10 MHz (reference)	600 MHz to 1.1 GHz	1.1 GHz to 1.6 GHz	1.6 GHz to 2.1 GHz
Amplitude Range (p-p)	5 mV to 3.5V			
1-Year Absolute Amplitude Uncertainty, tcal ± 5°C	±(2% of output + 300 μV)	±(7% of output + 300 μV)	±(7% of output + 300 μV)	±(8% of output + 300 μV)
Flatness (relative to 50 kHz)	Not applicable	±(5% of output + 100 μV)	±(5% of output + 100 μV)	±(6% of output + 100 μV)
Short-term Amplitude Stability	≤1% ¹			
Frequency Resolution	100 kHz			
1-Year Absolute Frequency, Uncertainty, tcal ± 5°C	±0.33 ppm			
2nd Harmonic	≤-33 dBc			
3rd and Higher Harmonics	≤-38 dBc			

¹ Within one hour after reference amplitude setting, provided temperature varies no more than ±5°C.

Time Marker Function

Time Marker into 50Ω	5s to 50 ms	20 ms to 100 ns (max)	50 ns to 20 ns	10 ns	5 ns to 2 ns	2 ns to 500 ps (2.1 GHz Option)
Wave Shape	spike or square	spike, square, or 20%-pulse	spike or square	square or sine	sine	sine
Sequence	5-2-1 from 5s to 2 ns (e.g., 500 ms, 200 ms, 100 ms)					
Period Resolution	4 digits					
1-Year Absolute Uncertainty, tcal ± 5°C	±(2.5 ppm + 5 μHz)	±0.33 ppm	±0.33 ppm	±0.33 ppm	±0.33 ppm	±0.33 ppm

Wave Generator

Wave Generator Characteristics	Sine and Square Wave into 50Ω or 1 MΩ	Triangle Wave into 50Ω or 1 MΩ
Amplitude Range	into 1 MΩ: 1.8 mV to 55V p-p; into 50Ω: 1.8 mV to 2.5V p-p	
1-Year Absolute Uncertainty, tcal ± 5°C, 10 Hz to 10 kHz	±(3% of p-p output + 100 μV)	
Sequence	1-2-5 (e.g., 10 mV, 20 mV, 50 mV)	
Typical DC Offset Range	0 to ±(≥40% of p-p amplitude) ¹	
Ramp Linearity		better than 0.1% 10 Hz to 10 kHz
Frequency Range	0.01 Hz to 100 kHz ²	
1-Year Absolute Uncertainty, tcal ± 5°C	±(2.5 ppm + 5 μHz)	

¹ The dc offset plus the wave signal must not exceed 30V rms.

² Sine wave to 500 kHz..

1 ns Pulse Generation

Pulse Generator Characteristics	Positive Pulse into 50Ω
Typical rise/fall times	≤500 ps
Typical Available Amplitudes	1.5V, 600 mV, 150 mV, 60 mV, 15 mV
Pulse Width Range	1 ns to 500 ns
Pulse Width Uncertainty	5% ± 200 ps
Pulse Period	20 ms to 200 ns
1-Year Absolute Uncertainty, tcal ± 5°C	± 0.33 ppm
Pulse Skew with Trigger Range	+30 ns to -10 ns with 250 ps resolution
Pulse Skew with Trigger Uncertainty	± 500 ps

Trigger Function

Available for pulse, time mark, edge and voltage functions.
TV Trigger is provided at the Output Terminal.

Trigger Signal Type	Parameters
Frame Formats	Selectable: NTSC, SECAM, PAL, PAL-M
Polarity	positive or negative
Line Marker	Selectable Line Video Marker

Tunnel Diode Drive Function

TD pulse drive	Square wave at 100 Hz to 100 kHz, with variable amplitude of 60V to 100V p-p
----------------	---

Current Output Function

	DC	Square Wave
Amplitude (compliance voltage 2V max)	± 100 μA to ± 100 mA	100 μA p-p to 100 mA p-p
Accuracy	± (0.25% + 0.5 μA)	± (0.25% + 0.5 μA) ¹
Frequency Range	N/A	10 Hz to 100 kHz
Accuracy		2.5 ppm + 5 μHz
Steps		1, 2, 5 or continuous

¹ Amplitude uncertainty for frequency range 45 Hz to 1 kHz at <120 mV compliance voltage.

Measurement Functions

Voltage Measurement		
DC Voltage Range ¹	± 10V	
DC Accuracy 0 to ±5.99V	0.05% + 1 mV	
DC Accuracy ±6 to ±10V	0.25% + 10 mV	
Resistance Measurement		
Measurement Range	40Ω to 60Ω and 500 kΩ to 1.5 MΩ	0.1%
Capacitance Measurement		
Measurement Range	5 pF to 50 pF	±(5% of input + 0.5 pF) ²

¹ Voltages exceeding 30 VDC may cause damage to the 5820A.

² Measurement made within 30 minutes of capacitance zero reference.

Auxiliary Input

Operates under the control of the 5820A. Frequency range up to 3 GHz.

Voltage rating 0-40V p-p. VSWR: <1.2:1 at 600 MHz; <1.5:1 at 2 GHz; <2.0:1 at 3 GHz.

General Specifications

Warm-up Time	Twice the time since last warmed up, to a maximum of 30 minutes
Settling Time	5 seconds or faster for all functions and ranges
Standard Interfaces	IEE-488 (GPIB), RS-232
Temperature Performance	Operating: 0 °C to 50 °C Calibration (tcal): 15 °C to 35 °C Storage: -20 °C to 70 °C
Electromagnetic Compatibility	Designed to operate in Standard Laboratory environments where the Electromagnetic environment is highly controlled. If used in areas with Electromagnetic fields > 1 V/m, there could be errors in current output values.
Temperature Coefficient	Temperature Coefficient for temperatures outside tcal ±5°C: add 0.1 x 1-year specification/°C
Relative Humidity	Operating: <80% to 30 °C, <70% to 40 °C, <40% to 50 °C Storage: <95%, non-condensing
Altitude	Operating: 3,050m (10,000 ft) maximum Non-operating: 12,200m (40,000 ft) maximum
Safety	Designed to comply with IEC 1010-1 (1992-1); ANSI/ISA-S82.01-1994; CAN/CSA-C22.2 No. 1010, 1-92
Analog Low Isolation	20V
EMC	Complies with EN 61326-1
Line Power	Line Voltage (selectable): 100V, 120V, 220V, 240V Line Frequency: 47 to 63 Hz Line Voltage Variation: ± 10% about line voltage setting
Power Consumption	250 VA
Dimensions	Height: 17.8 cm (7 in), standard rack increment, plus 1.5 cm (0.6 in) for feet on bottom of unit Width: 43.2 cm (17 in), standard rack width Depth: 47.3 cm (18.6 in) overall
Weight	20 kg (44 lb)

Ordering Information

Calibrators

5820A Oscilloscope Calibrator
 5500A Multi-Product Calibrator
 5520A High-Performance Multi-Product Calibrator

Options

2.1 GHz Bandwidth Extension for the 5820A
 Five Channel Output for the 5820A
 300 MHz Oscilloscope Calibration Option for the 5500A or 5520A
 600 MHz/300 ps Oscilloscope Calibration Option for the 5500A or 5520A

Upgrades

5800A-GHZK 2.1 GHz Bandwidth Extension Upgrade for Existing 5800As
 5820A-GHZK 2.1 GHz Bandwidth Extension Upgrade for Existing 5820As

Accessories

5800A/TDP 125 ps Tunnel Diode Pulser for the 5800A, 5820A and 5500A-SC600
 5500A/COIL 50-Turn Current Coil for the 5500A and 5520A
 5500A/CASE Transit Case with wheels for the 5500A, 5520A, 5800A and 5820A
 5500A/HNDL Side handle for the 5500A, 5520A, 5800A and 5820A
 Y5537 Rack mount kit for the 5500A, 5520A, 5800A and 5820A
 5500A/LEADS Comprehensive test lead kit for the 5500A and 5520A
 5800A-7004K Oscilloscope Cal Cable and Accessory Kit
 5800A-7002K Two Piece Replacement Output Cable Set
 5800A-7003K Five Piece Replacement Output Cable Set
 PM9581/011 Feed through Termination, 3W, 50 Ohm
 PM9584/021 Feed through T-Piece (matched power splitter), 50 Ohm
 PM 9061/001 Coupling, BNC (2x Female)
 PM9067/001 T-Piece, BNC (1 x Male 2 x Female)
 TC100 Test Cart

Software

MET/CAL-5 Automated Calibration and Asset Management
 5500/CAL-5 Automated Calibration and Asset Management for the 5500 and 5800 Series Calibrators
 MET/TRACK Metrology Asset Management

Fluke. *Keeping your world up and running.*

Fluke Corporation

PO Box 9090, Everett, WA USA 98206

Fluke Europe B.V.
 PO Box 1186, 5602 BD
 Eindhoven, The Netherlands

For more information call:

U.S.A. (800) 443-5853 or

Fax (425) 356-5116

Europe (31 40) 2 678 200 or

Fax (31 40) 2 678 222

Canada (905) 890-7600 or

Fax (905) 890-6866

Other countries (425) 356-5500 or

Fax (425) 356-5116

Web access: <http://www.fluke.com>

© 1999 Fluke Corporation. All rights reserved.
 Specifications subject to change without notice.
 Printed in U.S.A. 2/99 1268318

Printed on recycled paper.